


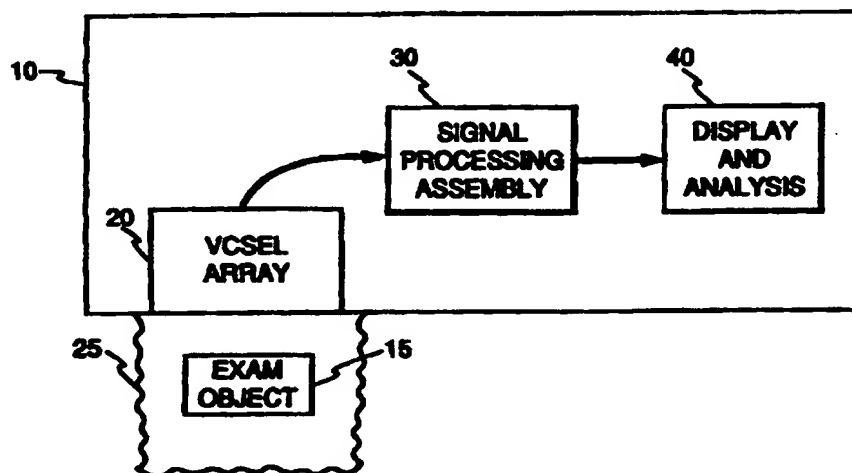

## INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification <sup>6</sup> : <b>G01H 9/00</b>	<b>A1</b>	(11) International Publication Number: <b>WO 96/30731</b> (43) International Publication Date: <b>3 October 1996 (03.10.96)</b>
(21) International Application Number: <b>PCT/US96/04026</b> (22) International Filing Date: <b>25 March 1996 (25.03.96)</b> (30) Priority Data: 08/414,833                31 March 1995 (31.03.95)                US (71) Applicant: <b>GENERAL ELECTRIC COMPANY [US/US]; 1 River Road, Schenectady, NY 12345 (US).</b> (72) Inventors: <b>DUGGAL, Anil, Raj; 1114 North Country Club Drive, Niskayuna, NY 12309 (US). YAKYMYSHYN, Christopher, Paul; Apartment 3, 4100 Grand Manor Court, Raleigh, NC 27612 (US).</b> (74) Agents: <b>STECKLER, Henry, I. et al.; General Electric Company, 3135 Easton Turnpike W3C, Fairfield, CT 06431 (US).</b>	(81) Designated States: <b>JP, European patent (AT, BE, CH, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE).</b> Published <i>With international search report.</i> <i>Before the expiration of the time limit for amending the claims and to be republished in the event of the receipt of amendments.</i>	

(54) Title: **ULTRASONIC DETECTOR USING VERTICAL CAVITY SURFACE EMITTING LASERS**

## (57) Abstract

An ultrasound/vibration detector array (10) includes an electrically pumped vertical cavity surface emitting laser (VCSEL) array (20). The cavity length of each laser or pixel for the array (20) is modulated by the acoustic field at the point where the acoustic field contacts the pixels. The resulting laser output is frequency modulated by the acoustic field. This modulation is converted to amplitude modulation at the detector head and then either detected with a charge-coupled-device (CCD) array with the information being electrically communicated to the signal processing assembly (30) or sent directly by optical fiber to the signal processing assembly (30) for processing. This ultrasound/vibration detector array (10) provides high frequency bandwidth detection, fine spatial resolution, and minimal electric cabling.

**FOR THE PURPOSES OF INFORMATION ONLY**

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AM	Armenia	GB	United Kingdom	MW	Malawi
AT	Austria	GE	Georgia	MX	Mexico
AU	Australia	GN	Guinea	NE	Niger
BB	Barbados	GR	Greece	NL	Netherlands
BE	Belgium	HU	Hungary	NO	Norway
BF	Burkina Faso	IE	Ireland	NZ	New Zealand
BG	Bulgaria	IT	Italy	PL	Poland
BJ	Benin	JP	Japan	PT	Portugal
BR	Brazil	KE	Kenya	RO	Romania
BY	Belarus	KG	Kyrgyzstan	RU	Russian Federation
CA	Canada	KP	Democratic People's Republic of Korea	SD	Sudan
CF	Central African Republic	KR	Republic of Korea	SE	Sweden
CG	Congo	KZ	Kazakhstan	SG	Singapore
CH	Switzerland	LI	Liechtenstein	SI	Slovenia
CI	Côte d'Ivoire	LK	Sri Lanka	SK	Slovakia
CM	Cameroon	LR	Liberia	SN	Senegal
CN	China	LT	Lithuania	SZ	Swaziland
CS	Czechoslovakia	LU	Luxembourg	TD	Chad
CZ	Czech Republic	LV	Latvia	TG	Togo
DE	Germany	MC	Monaco	TJ	Tajikistan
DK	Denmark	MD	Republic of Moldova	TT	Trinidad and Tobago
EE	Estonia	MG	Madagascar	UA	Ukraine
ES	Spain	ML	Mali	UG	Uganda
FI	Finland	MN	Mongolia	US	United States of America
FR	France	MR	Mauritania	UZ	Uzbekistan
GA	Gabon			VN	Viet Nam

- 1 -

**ULTRASONIC DETECTOR USING  
VERTICAL CAVITY SURFACE EMITTING  
LASERS**

**Background of the Invention**

5

This application is related to commonly assigned U.S. Pat. Application Serial No. \_\_\_\_\_, (RD-24,321) filed \_\_\_\_\_, 1995, of AR Duggal et al., filed concurrently herewith, the disclosure of which is hereby incorporated by reference.

10

This invention relates generally to imaging of acoustic energy, more particularly to laser-based ultrasound detection equipment and most particularly to an array of semiconductor microlaser-based ultrasound detection equipment.

15

Ultrasound equipment is commonly used in medical imaging and for non-destructive evaluation (NDE) of materials. Ultrasound analysis involves the propagation of energy through solids, liquids, and gases as acoustic waves; typically a pulse of acoustic energy is applied to an object to be imaged and reflected waves of the acoustic pulse are detected and processed for imaging and analysis. The spatial relationship and amplitude of the reflected waves provide information as to the location and nature of structures that reflected the acoustic energy in the object being analyzed.

20

Piezoelectric transducers are frequently used to generate ultrasound pulses transmitted into the object to be analyzed and to detect reflected waves received at the transducer. Piezoelectric devices require extensive electrical cabling which places practical limits on the number of pixels that can be placed in a transducer array, which in turn limits the resolution of the array.

25

Specifically, when utilizing piezoelectric transducers for ultrasound equipment used in medical imaging, currently a one-dimensional array of 128 elements or pixels are utilized. The piezoelectric pixels are each independently electrically connected by wires to the signal processing unit which would then process the signals received from the transducers to an imaging. In order to improve the ultrasound image quality, it is desired that a two-dimensional array with, such as, for example, 128 x 128 transducers/pixels is needed. Due to the

30

- 2 -

complexity of the many wires required to connect the piezoelectric transducers to the signal processor, and the complexity thereof, to utilize piezoelectric transducers is simply too complex.

Optical techniques have also been used for generation and  
5 detection of acoustic waves in ultrasound imaging. For example, energy from a laser beam focused on the surface of an object to be examined can generate an acoustic pulse in the object. The return pulse of acoustic energy is typically detected optically through the use of interferometry. A review of such techniques is provided in the book Laser Ultrasonics - Techniques and Applications by C.B.  
10 Scruby and L.E. Drain (IOP Publishing Ltd 1990), which is incorporated herein by reference. Noninterferometric techniques of optical detection of ultrasound include the knife-edge and surface-grating techniques and techniques based on reflectivity and light filters. See "Optical Detection of Ultrasound" by J.P. Monchalin, IEEE Transactions on Ultrasonics, Ferroelectrics, and Frequency  
15 Control, UFFC-33, September 1986, which is incorporated herein by reference. These laser-based methods of ultrasound detection are much less sensitive, by several orders of magnitude, than conventional piezoelectric-based methods.

Another laser-based method for detecting sound waves has been suggested in the article "Laser Hydrophone" by Y.A. Bykovskii et al., in Sov.  
20 Phys. Acoust. 34, p 204, March 1988. In the Bykovskii et al. optical hydrophone, movement of the hydrophone membrane varies the power and / or the phase of a semiconductor laser in the hydrophone to generate changes in the amplitude of an optical signal. The Bykovskii sonar hydrophone is relatively inefficient and thus has low sensitivity.

25 In a more recent approach to the use of an optical transducer assembly for ultrasound applications, an optical transducer assembly which includes a transducer housing and a signal laser, such as a microcavity laser or a microchip laser that is optically pumped, to detect ultrasound by monitoring the frequency modulation of the laser output caused by the interaction of the  
30 ultrasonic disturbance with the laser cavity, was mounted in the transducer housing. This interaction could involve a change in the laser cavity length and/or a change in the index of refraction of the lasing medium. This approach further detailed a scheme using fiber optic cables to reduce the interconnect complexity when using an array of microcavity lasers. The optical frequency generated by  
35 the signal laser is modulable (that is, adapted to or capable of being modulated)

- 3 -

in correspondence with acoustic energy incident on the transducer assembly. The signal laser comprises an optical cavity in which a lasing medium is disposed, and first and second reflectors that are disposed at respective opposite end surfaces of the optical cavity along an optical path axis of the cavity. The second  
5 reflector can alternatively be replaced with a compliant cavity that acts as a Gires-Tournois interferometer. The signal laser is adapted such that acoustic energy incident on the transducer assembly changes the length of a cavity along the optical path axis, or, alternatively, changes the index of refraction in the optical cavity, and such changes result in a substantially linear variation of the optical  
10 frequency of light generated by the laser.

In one embodiment, as disclosed in US Patent No. 5,353,262, assigned to the assignee of the present application, the disclosure of which is herein incorporated by reference, an optical transducer, such as used in an ultrasound system, includes a signal laser which generates an optical signal the  
15 frequency of which varies in correspondence with acoustic energy incident on the transducer. An optical cavity in the signal laser is disposed such that incident acoustic energy causes compression and rarefaction of the optical cavity, and this displacement varies optical frequency generated by the laser. A laser pump coupled to the lasing medium is adapted to apply selected levels of excitation  
20 energy appropriate to the detection of acoustic pulses. The signal laser alternatively is adapted such that the refractive index of the optical cavity is varied in correspondence with the incident acoustic energy to modulate the optical frequency of the light generated by the signal laser.

In an alternate embodiment, a piezoelectric device is disposed to  
25 receive the incident acoustic energy and generate a corresponding electrical signal that is applied to an electro-optic cell in the optical cavity, or alternatively, to conductors to generate an electric field across the lasing medium.

Despite the efforts described above to provide a simpler, more compact ultrasound detection device, a need still exists in medical imaging and  
30 nondestructive evaluation (NDE) of materials for an ultrasound transducer interfaced to support equipment which minimizes interconnection complexity. For example, as stated above, current state-of-the-art ultrasound imaging arrays use a linear array of about one hundred separate ultrasound pixels each of which are connected to a separate coaxial cable. Array sizes are currently limited by the  
35 complexity of the interconnect cabling. By using an optical interface between the

- 4 -

transducer head and support equipment, cabling can be significantly reduced in size for the same number of pixels. Alternatively, a much larger number of pixels can be connected by the same size cable. Additionally, it would be advantageous for NDE and underwater acoustic sensing applications to be able to detect as wide a frequency bandwidth of acoustic signals as possible. Finally, ultrasonic microscopic imaging of biological and micro-electronic structures requires an array of small, high bandwidth ultrasonic detectors in contact with the sample being imaged.

10

### Summary of the Invention

The ultrasound/vibration detector array of the present invention comprises an electrically pumped vertical cavity surface emitting laser (VCSEL) array. The cavity length of each laser or pixel of the array is modulated by the acoustic field at the point where the acoustic field contacts the pixels. The resulting laser output is frequency modulated by the acoustic field. This modulation is converted to amplitude modulation at the detector head and then either detected with a charge-coupled-device (CCD) array with the information being electrically communicated to the signal processing assembly or sent directly by optical fiber to the signal processing assembly for and processing. The ultrasound/vibration detector array of the present invention provides high frequency bandwidth detection, fine spatial resolution, and minimal electric cabling.

One embodiment of the present invention includes, a detector for detecting acoustic energy propagated through a medium, the detector comprising: a detector housing, and an electrically pumped vertical cavity surface emitting laser (VCSEL) array operatively positioned in the detector housing, each pixel of the array being a laser having a cavity length, the cavity length being modulated by an acoustic field.

Another embodiment of the present invention includes, an ultrasonic microscope comprising: an electrically pumped vertical cavity surface emitting laser (VCSEL) array operatively positioned in the detector housing, each pixel of the array being a laser having a cavity length, the cavity length being modulated by an acoustic field; an acoustic matching layer operatively positioned between the electrically pumped vertical cavity surface emitting laser (VCSEL) array and a sample to be imaged; a transparent acoustic backing layer

- 5 -

operatively connected to the VCSEL array, the VCSEL array generating an array of optical beams whose optical frequencies are modulated by the incident ultrasonic field, the beams being propagated through free space or Fiber-optic cabling; and a Fabry-Perot cavity array, operatively positioned relative to the backing layer but separated therefrom by free space or Fiber-optic cabling, for  
5 converting the frequency modulation of the laser output caused by the acoustic disturbance into amplitude modulation.

A still further embodiment of the present invention includes, an ultrasound system for analyzing a subject, comprising: a detector, and a signal  
10 processing assembly operatively connected to the detector, the optical detector comprising: a detector housing, and an electrically pumped vertical cavity surface emitting laser (VCSEL) array operatively positioned in the detector housing, each pixel of the array being a laser having a cavity length, the cavity length being modulated by an acoustic field.

15 It is accordingly an object of the present invention to provide a laser detector for detecting acoustic energy.

It is a further object of the present invention to provide a laser ultrasound system that is relatively compact.

It is another object of the present invention to provide a laser  
20 ultrasound detector having a large number of detector pixels in a compact detector array.

A still further object of the present invention is to provide a laser ultrasound detector that exhibits high sensitivity and a wide dynamic range.

Other objects and advantages of the invention will be apparent  
25 from the following description, the accompanying drawings and the appended claims.

#### Brief Description of the Drawings

30 Figure 1 is a block diagram of an ultrasound system comprising the present invention;

Figure 2 is a schematic diagram of an optical detector illustrating one embodiment of the present invention;

35 Figure 3 is a schematic diagram of an optical detector illustrating another embodiment of the present invention; and

- 6 -

Figure 4 is a schematic diagram of an optical detector illustrating yet a further embodiment of the present invention.

#### Detailed Description of the Invention

5

Figure 1 illustrates an ultrasound system 10 for analyzing an examination object 15 with acoustic energy comprising a detector 20, a signal processing assembly 30, and a display and analysis module 40. Detector 20 is acoustically coupled to object 15 through an acoustic couplant or matching layer 25 such that acoustic energy reflected from or transmitted through object 15 is received by detector 20.

In accordance with the present invention, detector 20 is adapted so that acoustic energy incident on the detector modulates the cavity length of each pixel of the electrically pumped vertical cavity surface emitting laser (VCSEL) array. This modulation is converted to optical frequency modulation of each pixel of the electrically pumped VCSEL which is in turn converted to optical amplitude modulation for each pixel. Detector 20 is in turn operatively connected to signal processing assembly 30 such that a processed output signal corresponding to the received acoustic energy is generated. Display and analysis module 40 is operatively connected to processing assembly 30 so that the processed output signal is visually presented or otherwise analyzed.

The present invention utilizes an array of vertical cavity surface emitting lasers (VCSEL's) or semiconductor microlasers to detect ultrasound by means of monitoring the frequency modulation of the laser output due to the interaction of the ultrasonic disturbance with each individual laser cavity. Each VCSEL array may contain, for example, about ten (10) to about ten thousand (10,000) or more individual microlasers or pixels as may be required or as can be fabricated by semiconductor processing methods.

Currently, considerable scientific research is being conducted in the characterization and improvement of VCSEL's. A useful description of the state of the art can be found in recent publications, one by Jewell et. al. "Vertical-Cavity Surface-Emitting Lasers: Design, Growth, Fabrication, Characterization", IEEE Journal of Quantum Electronics, 27 (1991) p. 1332 and one by Slusher "Semiconductor Microlasers and Their Applications", Optics & Photonics News, February 1993,p.8, the disclosure of each is incorporated herein by reference.



- 7 -

VCSEL's can be incorporated in acoustic detectors by a plurality of various arrangements. For example, two possible arrangements of incorporating VCSEL's in an acoustic detector in order to minimize electrical interconnects for the different pixels are shown schematically in figures 2 and 3.

5 Figure 2 illustrates one possible arrangement for detector 20 which uses optical fibers to communicate the output signal from each VCSEL pixel to the signal processing assembly. In this arrangement, the VCSEL array 42 is fabricated onto an acoustic matching layer 44 which is designed to allow maximum acoustic coupling into the detector assembly. An acoustic damping layer 46 is employed after the array 42 for extinguishing the acoustic energy in order to avoid reflections within the detector. Alternatively, an acoustic reflecting layer can be employed in place of the damping layer 46, depending on the sensitivity and bandwidth requirements of the specific application.

15 The frequency modulation of the laser output caused by the acoustic disturbance is then converted into amplitude modulation in a Fabry-Perot cavity array 48 or a single Fabry-Perot cavity attached to the damping layer 46. This cavity array 48 could also employ a spatial light modulator array or some other tuning element array which would allow feedback to correct for any laser fluctuations at frequencies lower than the acoustic frequency. Finally, an array of fiber optic couplers 50 would couple the amplitude modulated signal to the signal processing assembly 30.

25 Figure 3 illustrates a detector 20 arrangement which eliminates the need for the fiber optic bundle 50 to carry the signal information to the signal processing assembly 30. This arrangement is similar to that illustrated in Figure 2 except that the optical information is converted to electrical information at the detector head using a charge-coupled-device (CCD) array 52. By using a CCD or a combination of a few CCD's to image all the pixels, all the light-amplitude modulation information can be communicated back to the signal processing assembly 30 using only 1 or, at most, a few signal lines 54. In order to accomplish this, the CCD frame rate be fast compared to the acoustic frequency. Current state of the art CCD arrays have frame rates of greater than 100 KHz. Such CCD arrays should provide for successful analysis of acoustic frequencies up to about 50 KHz.

35 If the signal transmission rate from the CCD is high enough, it might be necessary to replace the electrical signal lines 54 with an optical fiber

- 8 -

using techniques known in the art of fiber optic communications in order to send the information to the signal processing assembly 30.

Figure 4 illustrates one possible arrangement for an ultrasonic microscope. A sample 56 to be imaged is in acoustic contact with the VCSEL array 42 by an acoustic impedance matching layer 44. The VCSEL array 42 generates an array of optical beams 60 whose optical frequencies are modulated by the incident ultrasonic field. An acoustic damping layer 46 is employed after the array 42 for extinguishing the acoustic energy in order to avoid reflections within the detector. Alternatively, an acoustic reflecting layer can be employed in place of the damping layer 46, depending on the sensitivity and bandwidth requirements of the specific application. The beams 60 are propagated to the previously described Fabry-Perot cavity array 48 and CCD array 52. The high frequency capability of a VCSEL allows high ultrasonic frequencies to be used resulting in superior spatial imaging resolution.

Detectors, in accordance with the present invention, are advantageously used in acoustic energy imaging systems such as ultrasound systems used for medical imaging or for non-destructive evaluation of materials, for ultrasonic microscopy and for undersea acoustic sensing.

The two most important distinguishing points for the purposes of the present invention are: (1) that an array of VCSEL's can be fabricated with a surface area for each laser or pixel on the order of about 10 microns squared and a cavity length on the order of about a few microns and (2) the lasers can be electrically pumped. The first distinguishing point implies that VCSEL acoustic detection allows extremely small pixels for two dimensional sensing arrays. Additionally, it can be shown that, for certain acoustic impedance matching layer combinations, the acoustic frequency detection bandwidth increases as the detecting laser cavity length decreases when the detection interaction involves a change in laser cavity length and the condition that the cavity length be much smaller than the acoustic wavelength holds. Thus, the small VCSEL cavity length leads to a high acoustic frequency detection bandwidth. The second point implies that the whole array can be powered by only two electrical lines.

While the systems and apparatus contained herein constitute preferred embodiments of the invention, it is to be understood that the invention is not limited to these precise systems and apparatus, and that changes may be

- 9 -

made therein without departing from the scope of the invention which is defined in the appended claims.

- 10 -

What is claimed is:

1. A detector for detecting acoustic energy propagated through a medium, the detector comprising:  
a detector housing, and  
an electrically pumped vertical cavity surface emitting laser  
5 (VCSEL) array operatively positioned in the detector housing, each pixel of the array being a laser having a cavity length, the cavity length being modulated by an acoustic field.
2. The detector of claim 1 wherein the resulting laser output is frequency modulated by the acoustic field.
3. The detector of claim 2 wherein the resulting laser output modulation is converted to amplitude modulation at the detector.
4. The detector of claim 3 wherein the amplitude modulation is detected with a CCD array, the information being electrically communicated to a signal processing assembly.
5. The detector of claim 3 wherein the amplitude modulation is sent directly to the signal processing assembly by optical fiber means.
6. The detector of claim 1 further comprising:  
an acoustic matching layer, operatively connected to the electrically pumped vertical cavity surface emitting laser (VCSEL) array, for allowing maximum acoustic coupling into the detector.
7. The detector of claim 1 further comprising:  
an acoustic damping layer operatively positioned after the electrically pumped vertical cavity surface emitting laser (VCSEL) array for extinguishing the acoustic energy in order to avoid reflections within the detector.
8. The detector of claim 1 further comprising:  
an acoustic reflecting layer operatively positioned after the electrically pumped vertical cavity surface emitting laser (VCSEL) array.
9. The detector of claim 7 further comprising:  
a Fabry-Perot cavity, operatively connected to the damping layer, for converting the frequency modulation of the laser output caused by the acoustic disturbance into amplitude modulation.
10. The detector of claim 9 further comprising:  
an array of fiber optic couplers for operatively connecting the amplitude modulated signal to a signal processing assembly.

- 11 -

11. The detector of claim 9 further comprising:  
means, operatively connected to the Fabry-Perot cavity, for  
converting optical information to electrical information.

12. The detector of claim 11 wherein the converting means  
comprises:

a charge-coupled-device (CCD) array.

13. The detector of claim 12 wherein, by using the (CCD)  
array or a combination of a few CCD's to image all the pixels, all the light-  
amplitude modulation information is communicated to the signal processing  
assembly using only 1 signal line.

14. An ultrasonic microscope comprising:

an electrically pumped vertical cavity surface emitting laser  
(VCSEL) array operatively positioned in the detector housing, each pixel of the  
array being a laser having a cavity length, the cavity length being modulated by  
5 an acoustic field;

an acoustic matching layer operatively positioned between the  
electrically pumped vertical cavity surface emitting laser (VCSEL) array and a  
sample to be imaged;

10 a transparent acoustic damping layer operatively connected to  
the VCSEL array, the VCSEL array generating an array of optical beams whose  
optical frequencies are modulated by the incident ultrasonic field, the beams  
being propagated through free space; and

15 a Fabry-Perot cavity, operatively positioned relative to the  
damping layer but separated therefrom, for converting the frequency modulation  
of the laser output caused by the acoustic disturbance into amplitude  
modulation.

15 The ultrasonic microscope of claim 14 further comprising:

a charge-coupled-device (CCD) array, operatively connected to  
the Fabry-Perot cavity.

16. An ultrasound system for analyzing a subject, comprising:  
a detector, and

a signal processing assembly operatively connected to the  
detector, the optical detector comprising:

5 a detector housing, and

- 12 -

an electrically pumped vertical cavity surface emitting laser (VCSEL) array operatively positioned in the detector housing, each pixel of the array being a laser having a cavity length, the cavity length being modulated by an acoustic field.

17. The system of claim 16 wherein the resulting laser output is frequency modulated by the acoustic field.

18. The system of claim 17 wherein the resulting laser output modulation is converted to amplitude modulation at the detector.

19. The system of claim 18 wherein the amplitude modulation is detected with a CCD array, the information being electrically communicated to a signal processing assembly.

20. The system of claim 16 further comprising:

an acoustic matching layer, operatively connected to the electrically pumped vertical cavity surface emitting laser (VCSEL) array, for allowing maximum acoustic coupling into the detector.

5

21. The system of claim 16 further comprising:

an acoustic damping layer operatively positioned after the electrically pumped vertical cavity surface emitting laser (VCSEL) array for extinguishing the acoustic energy in order to avoid reflections within the detector.

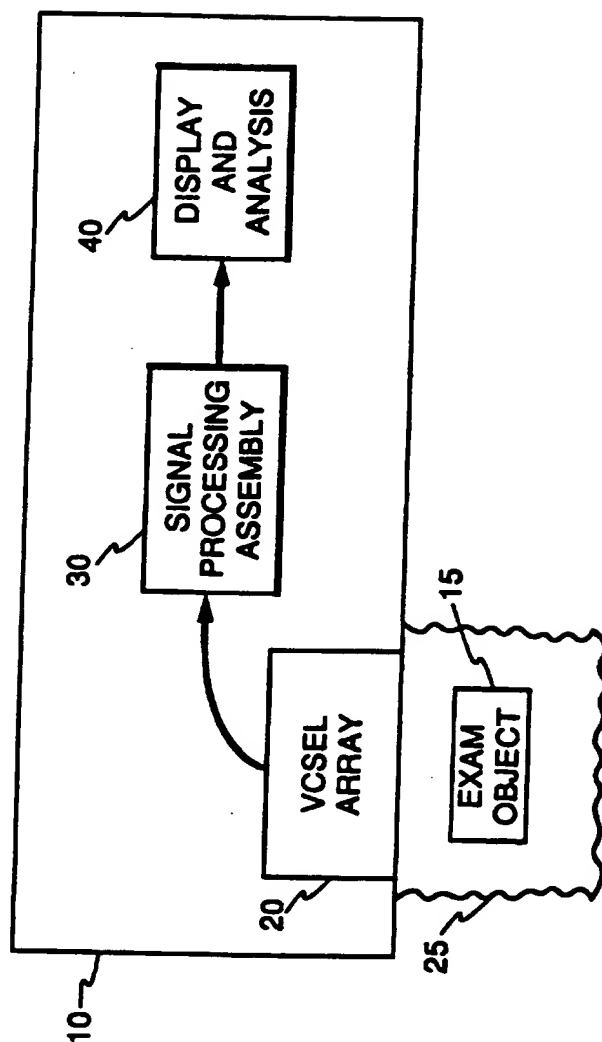


FIG. 1

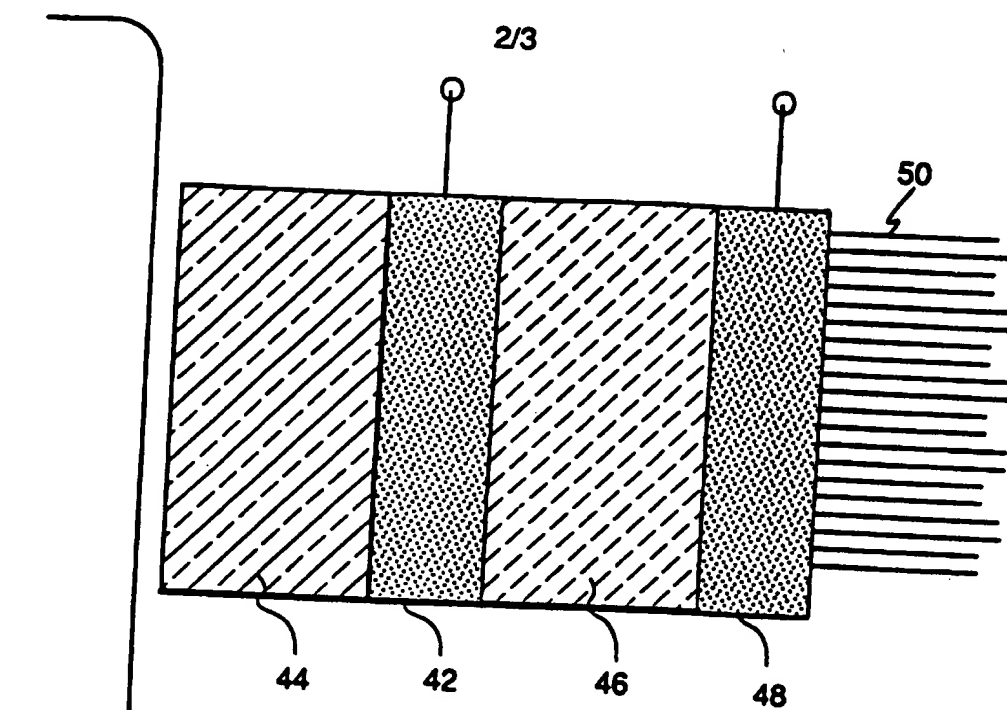


FIG. 2

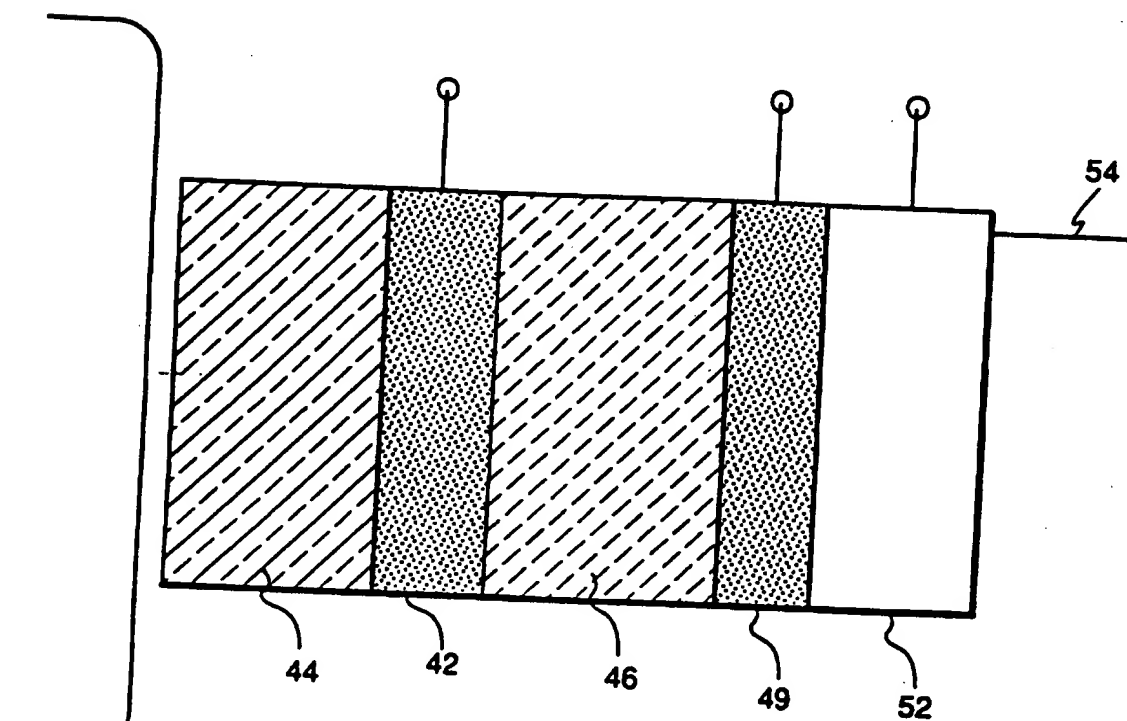


FIG. 3



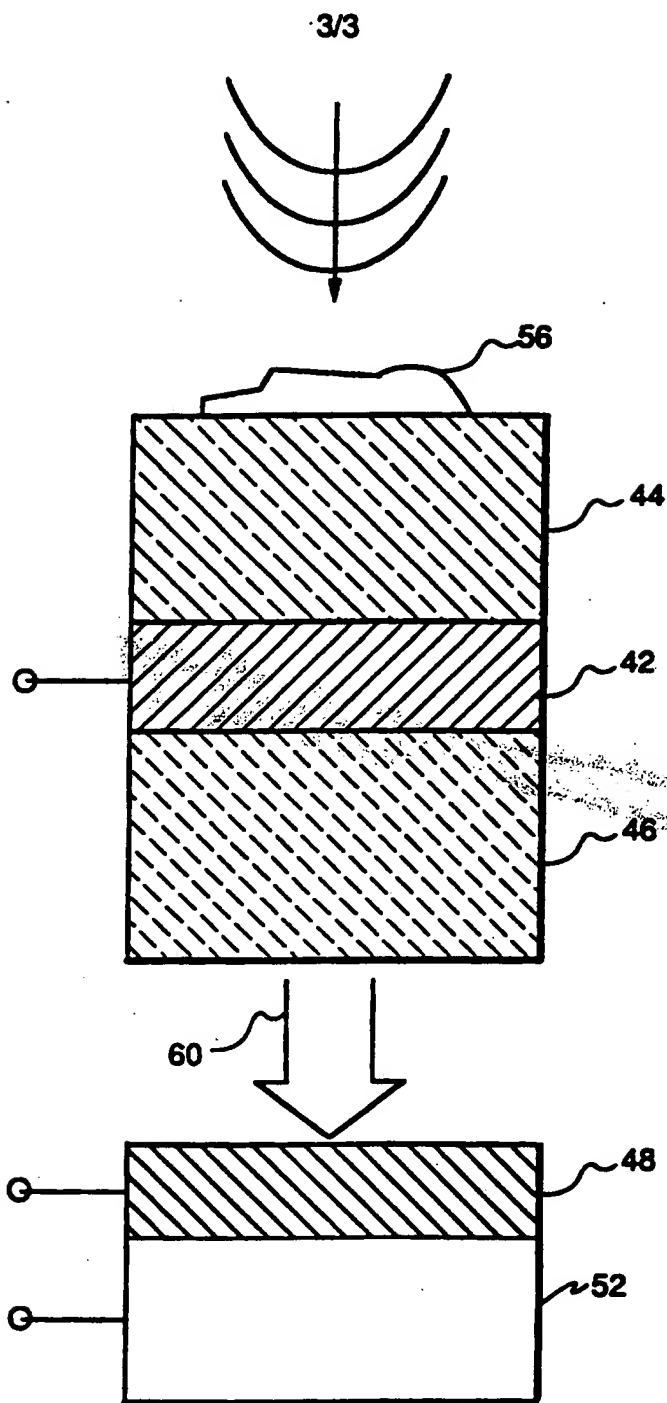


FIG. 4

# INTERNATIONAL SEARCH REPORT

Inter | ginal Application No  
PCT/US 96/04026

## A. CLASSIFICATION OF SUBJECT MATTER

IPC 6 G01H9/00

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 6 G01H

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US,A,5 331 658 (SHIEN CHAN-LONG ET AL) 19 July 1994 see abstract see column 1, line 7 - line 16 ---	1
A	IEEE JOURNAL OF QUANTUM ELECTRONICS, vol. 27, no. 6, 1 June 1991, pages 1332-1346, XP000229828 JEWELL J L ET AL: "VERTICAL-CAVITY SURFACE-EMITTING LASERS: DESIGN, GROWTH, FABRICATION, CHARACTERIZATION" cited in the application see page 1340, column 1, line 10 - line 18 ---	
A	US,A,4 546 458 (CIELO PAOLO G ET AL) 8 October 1985 see abstract; claim 1 ---	1
-/--		

☒ Further documents are listed in the continuation of box C.

☒ Patent family members are listed in annex.

### \* Special categories of cited documents:

- "A" document defining the general state of the art which is not considered to be of particular relevance
- "E" earlier document but published on or after the international filing date
- "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- "O" document referring to an oral disclosure, use, exhibition or other means
- "P" document published prior to the international filing date but later than the priority date claimed

- "T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- "X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- "Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.
- "A" document member of the same patent family

Date of the actual completion of the international search

30 July 1996

Date of mailing of the international search report

02.08.96

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2  
NL - 2280 HV Rijswijk  
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,  
Fax: (+31-70) 340-3016

Authorized officer

Anderson, A

# INTERNATIONAL SEARCH REPORT

Inter nal Application No

PCT/US 96/04026

## C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	<p>US,A,5 367 496 (SULLIVAN MICHAEL J ET AL)  22 November 1994  see claim 1</p> <p>-----</p>	1

# INTERNATIONAL SEARCH REPORT

Information on patent family members

Inter:      nal Application No

PCT/US 96/04026

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US-A-5331658	19-07-94	NONE	
US-A-4546458	08-10-85	CA-A- 1164950 GB-A,B 2100500	03-04-84 22-12-82
US-A-5367496	22-11-94	NONE	